




# Diagnostic accuracy of fecal calprotectin for screening patients with colorectal cancer: A meta-analysis

Xiaohua Ye<sup>1</sup> , Jiaping Huai<sup>2</sup> , Jin Ding<sup>1</sup> 

<sup>1</sup>Department of Gastroenterology, Jinhua Hospital of Zhejiang University, Jinhua, Zhejiang, China

<sup>2</sup>Department of Critical Care Medicine, Jinhua Hospital of Zhejiang University, Jinhua, Zhejiang, China

**Cite this article as:** Ye X, Huai J, Ding J. Diagnostic accuracy of fecal calprotectin for screening patients with colorectal cancer: A meta-analysis. *Turk J Gastroenterol* 2018; 29: 397-405.

## ABSTRACT

**Background/Aims:** Fecal calprotectin (FC) is reported to have a broad diagnostic accuracy for colorectal cancer (CRC). Therefore, we explored the diagnostic value of FC for CRC using meta-analytical techniques to substantiate the assertion.

**Materials and Methods:** An electronic search of the MEDLINE and Embase databases was conducted to identify studies that assessed the diagnostic accuracy of FC for CRC. The sensitivities and specificities of the eligible studies were summarized using a bivariable random-effects model.

**Results:** In total, 20 studies were included in the final analysis. The pooled sensitivity, specificity, positive likelihood ratio, and negative likelihood ratio of FC for CRC detection were 0.83 (95% confidence interval CI, 0.77-0.88), 0.61 (95% CI, 0.54-0.68), 2.15 (95% CI, 1.82-2.55), and 0.28 (95% CI, 0.21-0.37), respectively. The overall diagnostic odds ratio of FC for CRC was 7.76 (95% CI, 5.41-11.12) with an area under the curve of 0.81 (95% CI, 0.77-0.84), whereas the diagnostic value of FC for colorectal adenoma was relatively inferior (area under the curve, 0.55; 95% CI, 0.51-0.59; diagnostic odds ratio, 1.27; 95% CI, 0.91-1.78).

**Conclusion:** The results imply that the FC test, as currently implemented, cannot be recommended for CRC detection.

**Keywords:** Meta-analysis, calprotectin, colorectal cancer, diagnostic accuracy

## INTRODUCTION

Colorectal cancer (CRC) is the third most common malignancy worldwide and accounts for >10% of all cancer deaths (1). Based on the guidelines of the National Institute for Health and Care Excellence, serious pathology is predicted by clinical manifestations, including rectal bleeding, weight loss, and a change in bowel habits (1). However, these symptoms are not specific to CRC and hence have a rather low positive predictive value of 3%-4%, thereby precluding their utility for establishing a diagnosis of CRC (1). Although colonoscopy is considered the gold standard for early detection of CRC and its precursors (adenoma), this invasive and expensive method involves patient discomfort and potential complications (2). Therefore, a non-invasive screening method is needed to identify patients suspected of having CRC who otherwise would require colonoscopy.

Fecal calprotectin (FC) is a mucosal neutrophil degradation product, the presence of which appropriately correlates with bowel inflammation (2,3). FC is also a well-established biomarker of inflammatory bowel disease (1). Moreover, FC is associated other bowel diseases,

including CRC, adenoma, diverticulitis, and infectious diarrhea (4).

Colorectal cancer is associated with a local, acute inflammatory reaction of varying intensity. It is hypothesized that the local release of the chemotactic factor leads to the recruitment of neutrophils to the tumor site (4). A variety of inflammatory cells primarily along the invasive margin infiltrate human CRC tissue. Calprotectin activity is frequently detected in granulocytes and macrophages in CRC, and an increased numbers of granulocytes have been found in the feces of patients with CRC, likely because of shedding from the ulcerated tumor (5). Furthermore, it has been hypothesized that circulating leukocytes may actively migrate through neoplastic tissues in response to intraluminal antigens (5).

Numerous studies have evaluated the diagnostic accuracy of FC for the early detection of CRC. Despite the large body of evidence, conflicting results have raised concerns about the predictive value of FC for CRC detection across various patient populations. Indeed, a meta-analysis published in 2007 has revealed that FC is not suitable as a

ORCID IDs of the authors: X.Y. 0000-0002-8358-4093; J.H. 0000-0001-6778-6181; J.D. 0000-0002-5543-7969.

Corresponding Author: Jin Ding; dingjin@163.com

Received: September 30, 2017 Accepted: January 29, 2018 Available online date: May 30, 2018

© Copyright 2018 by The Turkish Society of Gastroenterology · Available online at [www.turkjgastroenterol.org](http://www.turkjgastroenterol.org)

DOI: 10.5152/tjg.2018.17606

screening test for CRC because of its relatively low diagnostic accuracy (6). After a decade, many new studies have been published regarding the diagnostic accuracy of FC for CRC. Thus, we conducted a systematic review and meta-analysis to update the current evidence.

## MATERIALS AND METHODS

### Search strategy

For our meta-analysis, we followed the Preferred Reporting Items for Systematic Reviews and Meta-analyses and guidelines from the Cochrane Diagnostic Test Accuracy Working Group (7). A computerized search of MEDLINE (from January 1, 1966 to December 31, 2016) and EMBASE (from January 1, 1974 to January 31, 2017) was performed to identify potentially relevant articles. The search was conducted using the following keywords: calprotectin ("calprotectin", "leukocyte L1 antigen complex", and "calgranulin"), colorectal ("colon", "rectal", "intestinal", and "bowel"), and cancer ("malignancy", "neoplasm", "tumor", and "adenoma"). In addition, the bibliographies from these potential articles were manually searched to identify additional studies. Citations were limited to those published in English. This work was approved by the Ethics Committee of our hospital. Informed consent was waived off because it was a meta-analysis.

### Study selection

Two reviewers (X.Y. and J.H.) independently reviewed potentially relevant articles for eligibility and inclusion. Studies were included if they met the following inclusion criteria: (1) prospective design published in a manuscript form; (2) patients for whom FC was used to detect CRC or colorectal adenoma; (3) an appropriate reference standard (endoscopy, radiology, or pathology) was included; (4) absolute numbers of true-positive, false-negative, true-negative, and false-positive observations for CRC and colorectal adenoma were reported or if data were sufficient to construct a 2×2 contingency table. Case reports, editorials, review articles, and clinical guidelines were excluded. Disagreements were resolved by a consensus.

### Data extraction and quality assessment

A custom-made standardized form was used for data extraction. The following data were extracted for each eligible study: the surname of the first author, publication year, location of the study population, study design, sample size (the number of patients with CRC or adenoma and the total number of subjects screened), details of the FC test (FC assay method, cut-off value), and a reference standard. The results were transformed by multiplying each value by a factor of 5, as previously confirmed, because some studies used a conventional assay to measure FC in terms of milligrams per liter (6-8).

The methodological qualities of the studies were assessed using the Quality Assessment of Diagnostic Accuracy Studies-2 (QUADAS-2) tool (9). QUADAS-2 consists of four key categories: patient selection, index test, reference standard, and flow and timing. Each category was assessed in terms of the risk of bias, and the first three categories were also considered to determine applicability.

### Data synthesis and statistical analysis

The 2×2 tables (numbers of true-positives, false-positives, true-negatives, and false-negatives) were constructed in accordance with the data from the included studies. The pooled estimates of sensitivity and specificity, positive likelihood ratio (PLR), negative likelihood ratio (NLR), and diagnostic odds ratio (DOR) were obtained using a bivariate random-effects model (10). Also, a hierarchical summary receiver-operating characteristic (HSROC) curve was produced to present the summary estimates of sensitivities and specificities along with their corresponding 95% confidence interval (CI) and prediction region. Moreover, the area under the HSROC curve (AUC) was calculated (11). The AUC and DOR values were used to evaluate the diagnostic efficacy of FC for the CRC and colorectal adenoma groups. A DOR of 1 implies that the test is incapable of determining whether a patient has a colorectal neoplasm. A higher value indicates better test performance.

Heterogeneity was evaluated using the Q-statistic and quantified using  $I^2$ . For the Q test, a p value of <0.10 was considered to imply heterogeneity. The value of  $I^2$  represents the proportion of total variation contributed by the between-study variation. The source of heterogeneity was explored using a threshold analysis, subgroup analysis, and meta-regression. Fagan plots were applied to illustrate the relationship among the prior test probability, PLR/NLR, and posterior test probability, and the Deek's test was used to evaluate publication bias (12). All statistical analyses were conducted using the STATA software version 12.0 (College Station; Texas, USA). A p value of <0.05 was considered to reflect statistical significance.

## RESULTS

### Study selection and characteristics

Our literature search identified 213 articles, of which 181 were then excluded upon an examination of the titles or abstracts because they were reviews, experimental studies, meta-analyses, comments, or other irrelevant articles (diagnostic studies of other biomarkers, letters, editorials, and consensus statements). Of the remaining 32 articles, 12 were subsequently excluded from the meta-analysis because two provided insufficient data to

construct a 2×2 table, five did not focus on the diagnostic study of interest, one did not have a control group, three were not prospective design, and one reported other cancers not relevant to CRC. As a result, 20 studies were identified for inclusion in our meta-analysis (Figure 1) (1-4,13-28).

Baseline characteristics of the 20 eligible studies are summarized in Table 1. These studies were published between 1993 and 2017 and were performed in seven regions. Of the 20 studies, 18 were conducted in Europe and two in

the USA. The number of participants in each study ranged from 80 to 2,321 and included a total of 427 cases with a diagnosis of CRC and 1,806 cases with a diagnosis of adenoma (one study presented 40 cases that described polyps) (13). Overall, six studies used the conventional FC assay, 12 used the new assay, one used both assay, and one did not specify the detection method (1-4,13-28). Based on the results from QUADAS-2, the study bias and applicability outcomes were assessed; the results are shown in supplementary Figure S1. Of the 20 studies, 11 were judged as high-risk in one or more of the four key categories.

### Diagnostic accuracy of the FC test

If multiple cut-off values or different assays for FC were reported in a single study, only the cut-off value or assay with the largest overall accuracy was used for the final analysis. Table 2 presents the results of the pooled sensitivity, specificity, AUC, and DOR of FC for distinguishing colorectal neoplasia. There were 18 studies that evaluated the diagnostic performance of FC for CRC detection (1-4, 13, 14, 16-21, 23-28). The pooled sensitivity and pooled specificity estimates were 0.83 (95% CI, 0.77-0.88) and 0.61 (95% CI, 0.54-0.68), respectively. Forest plots for pooled sensitivity and specificity are shown in Figure 2. The PLR and NLR values were 2.15 (95% CI, 1.82-2.55)

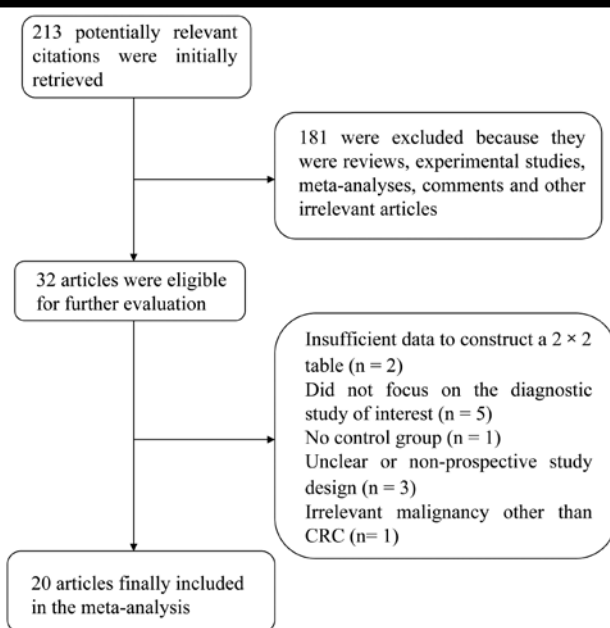


Figure 1. Flow chart for the selection of published studies for inclusion in our analysis

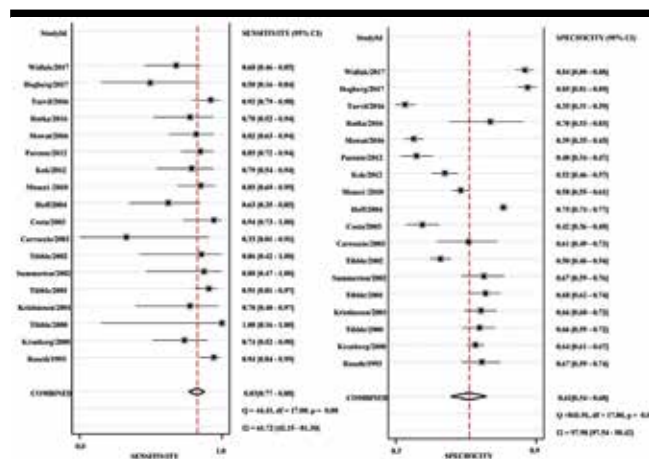


Figure 2. Forrest plots of sensitivity and specificity data for FC for CRC detection

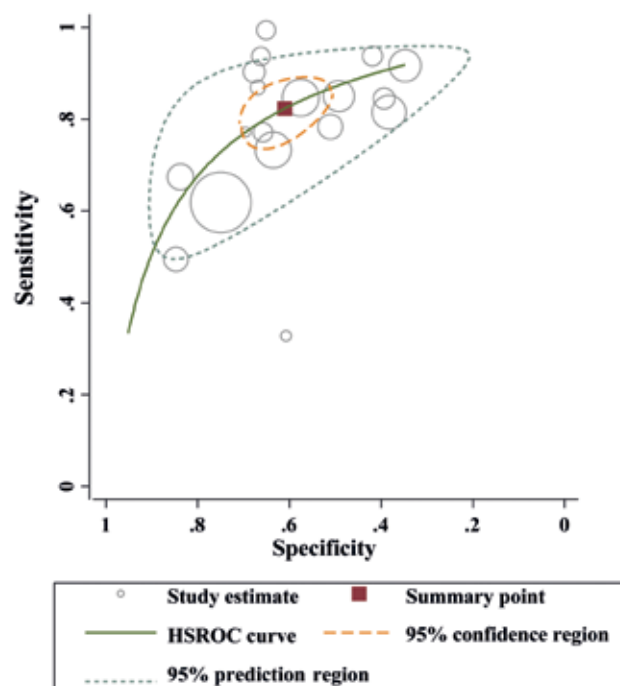


Figure 3. Hierarchical summary receiver-operating characteristic (HSROC) graph of the included studies that evaluated the diagnostic accuracy of FC for CRC detection

**Table 1.** Baseline characteristics of studies included in the meta-analysis

Author (year)	Region	Patient spectrum	Disease type	Sample size	No. of CRC	No. of adenomas	Assay	Reference standard	Cut-off
Roseth et al. (13) 1993	Norway	Known CRC, colorectal polyps	CRC, polyp	206	53	40 <sup>a</sup>	Roseth	Pathology, endoscopy	10 mg/L
Kronborg et al. (14) 2000	Europe	High-risk population for CRC	CRC, adenoma	814	23	203	PhiCal test	Pathology, endoscopy	10 mg/L
Limburg et al. (15) 2000	USA	Chronic diarrhea	Adenoma	110	-	21	PhiCal test	Pathology, endoscopy	100 µg/g
Tibble et al. (16) 2000	UK	Suspected inflammatory bowel disease	CRC, adenoma	220	2	3	Roseth	Pathology, endoscopy	10 mg/L
Kristinsson et al. (17) 2001	Norway	First-degree relatives of patients operated for CRC	CRC, adenoma	237	9 <sup>b</sup>	73	PhiCal test	Pathology, endoscopy	10 mg/L
Tibble et al. (4) 2001	UK	Suspected CRC	CRC, adenoma	295	66	29	Unclear	Pathology, endoscopy	10 mg/L
Summerton et al. (18) 2002	UK	Unselected patients with symptoms and/or signs	CRC, adenoma	134	8	6	PhiCal and Calprest ELISA	Pathology, endoscopy	10 mg/L 50 µg/g
Tibble et al. (19) 2002	UK	Suspected organic bowel disease	CRC	346	7	-	Roseth ELISA	Pathology, endoscopy	10 mg/L
Carroccio et al. (20) 2003	Italy	Chronic diarrhea	CRC	80	3 <sup>c</sup>	-	Calprest ELISA	Pathology, endoscopy	50 µg/g
Costa et al. (21) 2003	Italy	Outpatient clinic	CRC, adenoma	239	18 <sup>d</sup>	8	Calprest ELISA	Pathology, endoscopy, radiology	50 µg/g
Limburg et al. (22) 2003	USA	Suspected CRC	CRC, adenoma	412	3	94	PhiCal test	Pathology, endoscopy	50 µg/g
Hoff et al. (23) 2004	Norway	CRC screening in an average risk population	CRC, adenoma	2,321	16	787	PhiCal test	Pathology, endoscopy	50 µg/g
Meucci et al. (24) 2010	Italy	Unselected outpatients referred for colonoscopy	CRC, polyp	870	34	244	Calprest ELISA	Pathology, endoscopy	50 mg/dL
Kok et al. (25) 2012	Netherlands	Suspected organic bowel disease	CRC, adenoma	382	19	53	Calprotectin POC test	Pathology, endoscopy	50 µg/g
Parente et al. (26) 2012	Italy	Suspected CRC	CRC, adenoma	280	47	85	Calprotectin Buhlmann ELISA	Pathology, endoscopy	50 µg/g
Mowat et al. (1) 2016	UK	Suspected CRC	CRC, high-risk adenoma	755	28	41	Calprotectin EK-CAL	Pathology, endoscopy	50 µg/g
Rutka et al. (27) 2016	Hungary	Suspected CRC	CRC, adenoma	95	19	36	Quantum Blue ELISA	Pathology, endoscopy	Unclear

**Table 1.** Baseline characteristics of studies included in the meta-analysis (Continued)

Author (year)	Region	Patient spectrum	Disease type	Sample size	No. of CRC	No. of adenomas	Assay	Reference standard	Cut-off
Turvill et al. (3) 2016	UK	Suspected CRC	CRC, adenoma $\geq 10$ mm	654	39	33	EK-CAL Calprotectin ELISA	Pathology, endoscopy, radiology	50 $\mu\text{g/g}$
Högberg et al. (2) 2017	Sweden	Suspected CRC	CRC, high-risk adenoma	373	8	8	CALPROV® Calprotectin ELISA Test	Pathology, endoscopy	100 $\mu\text{g/g}$
Widlak et al. (28) 2017	UK	Suspected CRC	CRC, adenoma	430	25 <sup>b</sup>	42	ELISA Calprotectin immunoassay	Pathology	50 $\mu\text{g/g}$

<sup>a</sup>Described as "polyps"; adenomas with high-grade dysplasia were considered as CRC; <sup>c</sup>described as "colorectal cancer or adenomatous polyps"; included two cases with colorectal lymphoma  
 CRC: colorectal cancer; ELISA: enzyme-linked immunosorbent assay

**Table 2.** Diagnostic performance of FC for colorectal neoplasia

	CRC vs. non-CRC	Adenoma vs. non-adenoma
Number of patients	8,913	7,662
Sensitivity (95% CI)	0.83 (0.77, 0.88)	0.49 (0.37, 0.61)
I2 (%)	61.72%	92.79%
Specificity (95% CI)	0.61 (0.54, 0.68)	0.57 (0.49, 0.65)
I2 (%)	97.98%	97.84%
PLR (95% CI)	2.15 (1.82, 2.55)	1.14 (0.96, 1.35)
I2 (%)	87.24%	91.76%
NLR (95% CI)	0.28 (0.21, 0.37)	0.90 (0.76, 1.06)
I2 (%)	64.99%	84.97%
AUC (95% CI)	0.81 (0.77, 0.84)	0.55 (0.51, 0.59)
I2 (%)	96%	99%
DOR (95% CI)	7.76 (5.41, 11.12)	1.27 (0.91, 1.78)
I2 (%)	97.97%	100.00%

FC: fecal calprotectin; CI: confidence interval; PLR: positive likelihood ratio; NLR: negative likelihood ratio; AUC: area under the HSROC curve; DOR: diagnostic odds ratio; HSROC: hierarchical summary receiver-operating characteristic

and 0.28 (95% CI, 0.21-0.37), respectively, and the AUC and DOR values were 0.81 (95% CI, 0.77-0.84) and 7.76 (95% CI, 5.41-11.12), respectively (Figure 3).

Of the 20 eligible studies, 15 (1-4, 13-17, 21-23, 25, 26, 28) evaluated the diagnostic accuracy of FC for colorectal adenoma. For adenoma, the overall pooled sensitivity, specificity, PLR, and NLR for FC were 0.49 (95% CI, 0.37-0.61), 0.57 (95% CI, 0.49-0.65), 1.14 (95% CI, 0.96-1.35), and 0.90 (95% CI, 0.76-1.06), respectively. The average AUC and DOR values for adenoma were 0.55 (95% CI, 0.51-0.59) and 1.27 (95% CI, 0.91-1.78), respectively.

Overall, these results suggested that the utility of FC for detecting colorectal adenoma was insufficient for clinical application (Table 2).

### Publication bias

Deek's funnel plot asymmetry and the results of the Deek's test ( $p=0.204$  for CRC,  $p=0.407$  for adenoma) did not suggest any potential publication bias (Figure 4).

### Investigation of heterogeneity

Our results were heterogeneous (Table 2). We first performed a Spearman analysis and found that there was no threshold effect within the studies ( $r=0.451$ ,  $p=0.060$ ). We also performed subgroup analyses to detect the source of heterogeneity based on patient spectrum, FC assay method, prevalence, sample size, publication year, and cut-off value. Synthesized data revealed that the heterogeneity did not significantly change with variations in the patient spectrum (Table 3). CRC detection by the conventional FC assay exhibited greater sensitivity than the new assay, as evidenced by the reduced heterogeneity ( $I^2=37.42\%$ ) and an increased DOR value of 12.15 (5.67, 26.05). Therefore, the assay by which FC was measured appeared to significantly contribute to the heterogeneity. Probably, the performance characteristics of FC for CRC detection were considerably better in studies with a higher level of prevalence (above the average) and a smaller sample size (below the median). However, the diagnostic performance remained similar and the heterogeneity did not notably decrease with respect to the publication year or cut-off value (Table 3). We also performed meta-regression to identify any significant sources of heterogeneity (Figure S2). The patient spectrum ( $p<0.01$ ), FC assay ( $p<0.001$ ), sample size ( $p<0.001$ ), and publication year ( $p<0.001$ ) significantly contributed to the heterogeneity in sensitivity. However, the cut-off value ( $p<0.05$ ) accounted for heterogeneity in specificity.

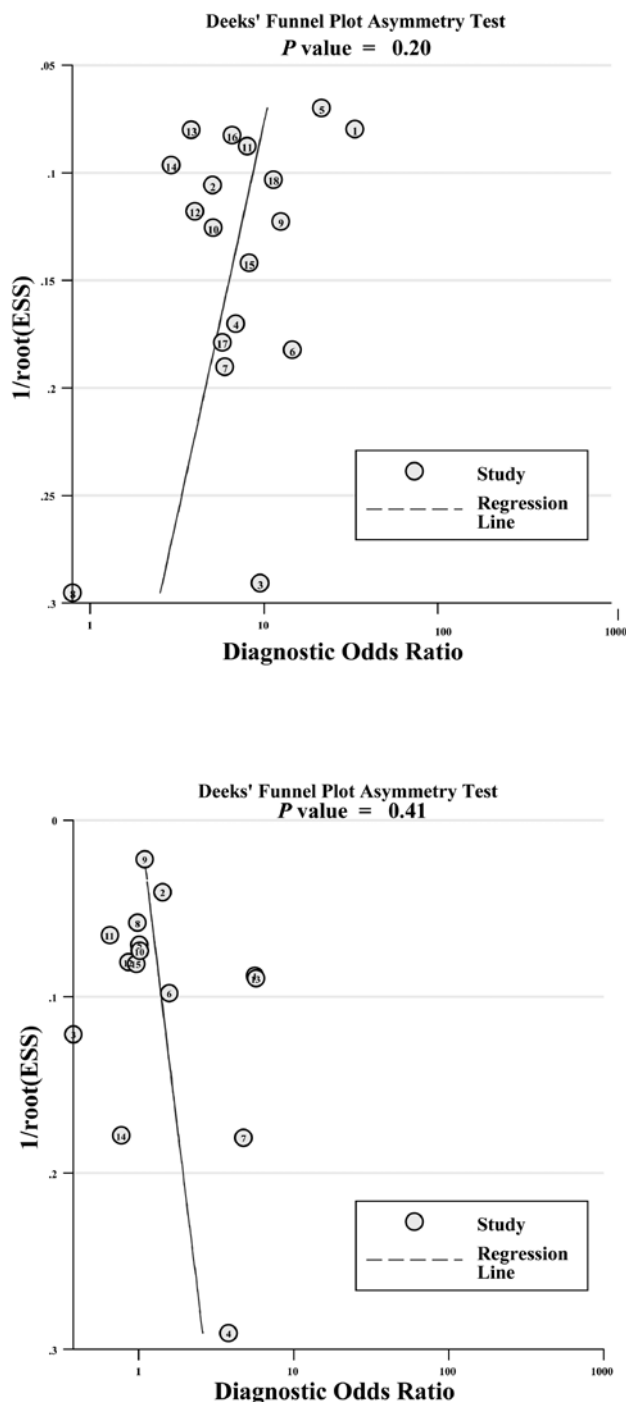


Figure 4. Funnel plot with superimposed regression line for studies of (A) CRC and (B) colorectal adenoma

### Predictive value of the FC test

The Fagan plot was applied to assess the clinical utility of the FC test for predicting CRC in the screened populations (Figure S3). The diagnosis of CRC was confirmed in 4.6% ( $n=427$ ) of the total included patients ( $n=9,253$ ). Consequently, with a pretest probability of 4.6%, a positive FC test was found to predict an increase in the risk of CRC to 10%; conversely, a negative FC test was found to decrease the risk of CRC to 1%.

### DISCUSSION

In this study, we conducted a robust systematic review and meta-analysis. The results showed that the pooled sensitivity and specificity values of FC for CRC were approximately 83% and 61%, respectively. In addition, the overall accuracy of FC for predicting CRC was 81%. With regard to colorectal adenoma, the FC test is of inferior diagnostic value as assessed by our quantitative analysis (AUC, 0.55; 95% CI, 0.51-0.59; DOR, 1.27; 95% CI, 0.91-1.78).

The latest systematic review was published in 2007, which included 12 studies with respect to the diagnostic accuracy of FC for colorectal neoplasia (6). Our present analysis included 20 studies and it updates the body of evidence. The prior systematic review combined CRC and adenoma together as "neoplasia" and concluded that FC was not suitable for CRC screening. Our study differs in that we analyzed each case of CRC and adenoma. Nevertheless, our results suggest that the FC test, as it currently exists, cannot be recommended for CRC detection.

The diagnosis of CRC can be challenging for gastroenterologists because of its nonspecific symptoms. At present, the majority of referred cases from primary care for evaluation of bowel symptoms undergo invasive tests including colonoscopy, but the diagnosis of pathology is low (1). For example, currently, only 8% of patients who complain of bowel symptoms receive a confirmed diagnosis of CRC (3). Also, functional gastrointestinal disorders, including irritable bowel syndrome, are often found to coexist in 75% of symptomatic patients (as assessed with colonoscopy), and such conditions respond well to the typical treatment (3,26). However, colonoscopy is an invasive, expensive procedure with an established risk of complications. Moreover, there is limited availability of colonoscopy services in many regions of the world; thus, colonoscopy screening should be reserved for higher risk individuals to optimize resource utilization (26). Therefore, a non-invasive and simple test may be preferable for prioritizing referrals for colonoscopy. The fecal occult blood test has been widely used as a preliminary assessment, and it has been shown to reduce disease-specific mortality; however, its accuracy is affected by the dietary pattern, and nearly 50% of

**Table 3.** Subgroup analyses of FC for CRC detection

Subgroup	No. of studies	Sensitivity (95% CI)	Specificity (95% CI)	PLR (95% CI)	NLR (95% CI)	AUC (95% CI)	DOR (95% CI)
<i>Patient spectrum</i>							
Suspected CRC	9	0.81 (0.73, 0.88)	0.63 (0.49, 0.75)	2.19 (1.63, 2.96)	0.30 (0.21, 0.41)	0.81 (0.78, 0.84)	7.42 (4.66, 11.82)
<i>I</i> <sup>2</sup> (%)		69.72%	98.61%	93.16%	69.54%	96%	99.60%
Others	8	0.85 (0.73, 0.92)	0.59 (0.52, 0.66)	2.09 (1.76, 2.48)	0.25 (0.14, 0.45)	0.76 (0.72, 0.80)	8.28 (4.21, 16.26)
<i>I</i> <sup>2</sup> (%)		62.87%	97.76%	49.09%	69.17%	80%	96.00%
<i>FC assay</i>							
Old	6	0.88 (0.78, 0.93)	0.63 (0.58, 0.68)	2.39 (1.98, 2.87)	0.20 (0.11, 0.36)	0.80 (0.77, 0.84)	12.15 (5.67, 26.05)
<i>I</i> <sup>2</sup> (%)		37.42%	90.38%	10.33%	41.39%	0%	90.99%
New	9	0.78 (0.68, 0.86)	0.59 (0.45, 0.72)	1.92 (1.47, 2.50)	0.36 (0.27, 0.49)	0.77 (0.73, 0.81)	5.30 (3.55, 7.93)
<i>I</i> <sup>2</sup> (%)		76.48%	99.00%	90.80%	76.68%	97.00%	96.97%
<i>Prevalence</i>							
>average	9	0.87 (0.81, 0.92)	0.59 (0.48, 0.70)	2.14 (1.66, 2.77)	0.21 (0.15, 0.31)	0.85 (0.82, 0.88)	10.07 (6.04, 16.77)
<i>I</i> <sup>2</sup> (%)		58.07%	97.59%	90.89%	52.41%	93%	98.93%
<average	9	0.75 (0.64, 0.83)	0.64 (0.54, 0.72)	2.07 (1.68, 2.53)	0.40 (0.29, 0.55)	0.76 (0.72, 0.79)	5.22 (3.41, 7.99)
<i>I</i> <sup>2</sup> (%)		40.98%	98.26%	61.72%	48.60%	92%	83.80%
<i>Sample size</i>							
>median	9	0.78 (0.68, 0.86)	0.62 (0.49, 0.73)	2.06 (1.59, 2.67)	0.35 (0.26, 0.47)	0.78 (0.74, 0.82)	5.87 (3.98, 8.65)
<i>I</i> <sup>2</sup> (%)		61.02%	98.93%	89.60%	45.95%	96%	91.34%
<median	9	0.88 (0.84, 0.92)	0.61 (0.53, 0.68)	2.25 (1.85, 2.74)	0.19 (0.13, 0.28)	0.89 (0.86, 0.91)	11.86 (6.87, 20.47)
<i>I</i> <sup>2</sup> (%)		52.74%	90.99%	78.89%	71.70%	35%	99.71%
<i>Publication year</i>							
Before 2007	10	0.86 (0.76, 0.92)	0.63 (0.57, 0.69)	2.33 (2.00, 2.70)	0.22 (0.13, 0.39)	0.78 (0.74, 0.82)	10.49 (5.59, 19.72)
<i>I</i> <sup>2</sup> (%)		60.69%	96.25%	54.46%	68.24%	83%	93.57%
After 2007	8	0.80 (0.71, 0.87)	0.60 (0.44, 0.73)	1.99 (1.47, 2.69)	0.33 (0.25, 0.44)	0.79 (0.76, 0.83)	6.00 (3.88, 9.28)
<i>I</i> <sup>2</sup> (%)		66.65%	98.64%	91.38%	60.78%	96%	97.75%
<i>Cut-off value</i>							
50 µg/g or 10 mg/L	15	0.84 (0.78, 0.89)	0.59 (0.51, 0.67)	2.06 (1.73, 2.45)	0.27 (0.19, 0.37)	0.81 (0.77, 0.84)	7.71 (5.06, 11.76)
<i>I</i> <sup>2</sup> (%)		60.61%	98.12%	87.29%	65.00%	95%	97.56%
Others	3	-	-	-	-	-	-
<i>I</i> <sup>2</sup> (%)		-	-	-	-	-	-

AUC: area under the HSROC curve; FC: fecal calprotectin; CI: confidence interval; CRC: colorectal cancer; PLR: positive likelihood ratio; NLR: negative likelihood ratio; DOR: diagnostic odds ratio; HSROC: Hierarchical summary receiver-operating characteristic

colonoscopies performed based on a positive fecal occult blood test result show no evidence of neoplasia (26). Indeed, previous studies have supported the use of the fecal immunohistochemical test (FIT) for CRC screening in average-risk populations because of its high accuracy and reproducibility (29). FC is stable in stools because of its resistance to bacterial degradation at room temperature for up to 7 days, and studies have found that the sensitivity of the FC test for detecting CRC ranges from 79% to 95% (2). However, our data suggest that the FC test alone is not powerful enough to screen for CRC. Therefore, we infer that there is probably no place for FC as a screening tool for CRC in average-risk populations.

Although the FC test cannot be recommended as the sole screening modality for CRC, our data still have clinical implications. We propose that FC should be used as an auxiliary tool to help clinicians stratify CRC risk in different patients because the FC test may help predict CRC development. Nevertheless, significant risk factors associated with CRC, such as age, gender, anemia, family history of cancer, and change of bowel movement habits, should also be considered when planning further treatment. Indeed, previously reported preliminary results substantiated the benefit of the FC test in a diagnostic model of significant colorectal disease (including CRC) (30). It is thus imperative that future studies include larger and better-defined patient populations.

There was significant heterogeneity among some of our results. We selected studies with a prospective design and excluded case-control studies because they tend to overestimate the diagnostic precision. Therefore, the heterogeneity caused by the study design was largely avoided. We used a random-effects model, which assumed that the true effects were normally distributed, and more weightage was assigned to the small-sized studies compared with the fixed-effects model. Subgroup analyses were also conducted to address heterogeneity (Table 3). However, the subgroup summary estimates did not differ significantly from the overall summary estimates, suggesting that the overall summary measures reflect the reasonable estimations of the overall FC test accuracy despite some statistical heterogeneity. Selection bias was likely to be another source of heterogeneity because numerous different diagnoses were grouped together in some of our analyses. For instance, the non-CRC group or non-adenoma group contained patients with diverse gastrointestinal conditions, such as inflammatory bowel disease, diverticulosis, food intolerance, and irritable bowel syndrome, as well as healthy controls. Nonetheless, this phenomenon reflects a "real world" scenario and therefore provides a realistic estimation of the CRC risk.

Moreover, meta-regression was used to decipher the nature of heterogeneity. Patient spectrum, FC assay method, sample size, publication year, and cut-off value were identified as potential confounding factors that may have contributed to the heterogeneity.

Some limitations of our study merit consideration. First, the FC assay varied across studies, and this affected our interpretation of the analyses. Second, we could not determine the sensitivity and specificity of FC for CRC stratified by disease site (proximal or distal) or cancer stage because of a paucity of relevant data. Third, few studies focused on the value of simultaneously or consecutively administering patients with other tests. For example, Mowat et al. (1) found FIT to be superior to FC, whereas others found a similar negative predictive value when comparing FC and FIT (25,26). Overall, three studies assessed the value of the combination of FC and FIT for detecting CRC but showed no significant improvement in the diagnostic accuracy (1,2,28). However, the resolution of this issue will require more data and additional studies. These approaches could aid clinicians to maximize the use of FC and other biomarkers in clinical practice. Fourth, our study could not derive a summarized estimation of the performance of FC for advanced adenoma because the definition of advanced adenoma varied across studies. Finally, the absence of data from Asia may compromise the results. Several of the included studies were conducted in primary care facilities. However, in Asia, particularly mainland China, the public prefers to select hospital-based services instead of community-based primary care against a background of the "bare-foot doctor" legacy in rural China and hence, a mistrust of doctors. China has the largest population in the world; however, cancer surveillance needs improvement, and the availability of endoscopy in secondary-care facilities lags far behind other areas of the world. Therefore, studies are needed to address this deficiency.

In summary, the FC test was found to be unsuitable for screening CRC. Whether the combination of FC and other biomarkers would enhance CRC detection needs further investigation. Moreover, studies from Asia are urgently needed.



You can reach the supplemental figures of this article at <https://10.5152/tjg.2018.17606>

**Ethics Committee Approval:** Ethics committee approval was received for this study from the Ethics Committee of Zhejiang University Jinhua Hospital.



**Informed Consent:** N/A.

**Peer-review:** Externally peer-reviewed.

**Author Contributions:** Concept - X.Y.; Design - J.D.; Supervision - J.D.; Resource - J.D.; Materials - J.H.; Data Collection and/or Processing - J.H.; Analysis and/or Interpretation - X.Y.; Literature Search - X.Y.; Writing - X.Y. Critical Reviews - J.D.

**Conflict of Interest:** The authors have no conflict of interest to declare.

**Financial Disclosure:** This study was funded by two grants from Key Research Projects of Jinhua Municipal Technology Bureau (Grant No. 2013-3-010) and the Science and Technology Bureau of Jinhua, Zhejiang Province, China (Grant No. 2014-3-053).

## REFERENCES

- Mowat C, Digby J, Strachan JA, et al. Faecal haemoglobin and faecal calprotectin as indicators of bowel disease in patients presenting to primary care with bowel symptoms. *Gut* 2016; 65: 1463-9. [CrossRef]
- Hogberg C, Karling P, Rutegard J, Lilja M. Diagnosing colorectal cancer and inflammatory bowel disease in primary care: The usefulness of tests for faecal haemoglobin, faecal calprotectin, anaemia and iron deficiency. A prospective study. *Scand J Gastroenterol* 2017; 52: 69-75. [CrossRef]
- Turvill J, Aghahoseini A, Sivarajasingham N, et al. Faecal calprotectin in patients with suspected colorectal cancer: a diagnostic accuracy study. *Br J Gen Pract* 2016; 66: e499-506. [CrossRef]
- Tibble J, Sigthorsson G, Foster R, Sherwood R, Fagerhol M, Bjarnason I. Faecal calprotectin and faecal occult blood tests in the diagnosis of colorectal carcinoma and adenoma. *Gut* 2001; 49: 402-8. [CrossRef]
- Lehmann FS, Trapani F, Fueglistaler I, et al. Clinical and histopathological correlations of fecal calprotectin release in colorectal carcinoma. *World J Gastroenterol* 2014; 20: 4994-9. [CrossRef]
- von Roon AC, Karamountzos L, Purkayastha S, et al. Diagnostic precision of fecal calprotectin for inflammatory bowel disease and colorectal malignancy. *Am J Gastroenterol* 2007; 102: 803-13. [CrossRef]
- Leeftang MM, Deeks JJ, Gatsonis C, Bossuyt PM, Cochrane Diagnostic Test Accuracy Working G. Systematic reviews of diagnostic test accuracy. *Ann Intern Med* 2008; 149: 889-97. [CrossRef]
- Lin JF, Chen JM, Zuo JH, et al. Meta-analysis: fecal calprotectin for assessment of inflammatory bowel disease activity. *Inflamm Bowel Dis* 2014; 20: 1407-15. [CrossRef]
- Whiting PF, Rutjes AW, Westwood ME, et al. QUADAS-2: a revised tool for the quality assessment of diagnostic accuracy studies. *Ann Intern Med* 2011; 155: 529-36. [CrossRef]
- Reitsma JB, Glas AS, Rutjes AW, Scholten RJ, Bossuyt PM, Zwinderman AH. Bivariate analysis of sensitivity and specificity produces informative summary measures in diagnostic reviews. *J Clin Epidemiol* 2005; 58: 982-90. [CrossRef]
- Rutter CM, Gatsonis CA. A hierarchical regression approach to meta-analysis of diagnostic test accuracy evaluations. *Stat Med* 2001; 20: 2865-84. [CrossRef]
- Deeks JJ, Macaskill P, Irwig L. The performance of tests of publication bias and other sample size effects in systematic reviews of diagnostic test accuracy was assessed. *J Clin Epidemiol* 2005; 58: 882-93. [CrossRef]
- Roseth AG, Kristinsson J, Fagerhol MK, et al. Faecal calprotectin: a novel test for the diagnosis of colorectal cancer? *Scand J Gastroenterol* 1993; 28: 1073-6. [CrossRef]
- Kronborg O, Ugstad M, Fuglerud P, et al. Faecal calprotectin levels in a high risk population for colorectal neoplasia. *Gut* 2000; 46: 795-800. [CrossRef]
- Limburg PJ, Ahlquist DA, Sandborn WJ, et al. Fecal calprotectin levels predict colorectal inflammation among patients with chronic diarrhea referred for colonoscopy. *Am J Gastroenterol* 2000; 95: 2831-7. [CrossRef]
- Tibble J, Teahon K, Thjodleifsson B, et al. A simple method for assessing intestinal inflammation in Crohn's disease. *Gut* 2000; 47: 506-13. [CrossRef]
- Kristinsson J, Nygaard K, Aadland E, et al. Screening of first degree relatives of patients operated for colorectal cancer: evaluation of fecal calprotectin vs. hemoccult II. *Digestion* 2001; 64: 104-10. [CrossRef]
- Summerton CB, Longlands MG, Wiener K, Shreeve DR. Faecal calprotectin: a marker of inflammation throughout the intestinal tract. *Eur J Gastroenterol Hepatol* 2002; 14: 841-5. [CrossRef]
- Tibble JA, Sigthorsson G, Foster R, Forgacs I, Bjarnason I. Use of surrogate markers of inflammation and Rome criteria to distinguish organic from nonorganic intestinal disease. *Gastroenterology* 2002; 123: 450-60. [CrossRef]
- Carroccio A, Iacono G, Cottone M, et al. Diagnostic accuracy of fecal calprotectin assay in distinguishing organic causes of chronic diarrhea from irritable bowel syndrome: a prospective study in adults and children. *Clin Chem* 2003; 49: 861-7. [CrossRef]
- Costa F, Mumolo MG, Bellini M, et al. Role of faecal calprotectin as non-invasive marker of intestinal inflammation. *Dig Liver Dis* 2003; 35: 642-7. [CrossRef]
- Limburg PJ, Devens ME, Harrington JJ, Diehl NN, Mahoney DW, Ahlquist DA. Prospective evaluation of fecal calprotectin as a screening biomarker for colorectal neoplasia. *Am J Gastroenterol* 2003; 98: 2299-305. [CrossRef]
- Hoff G, Grotmol T, Thiis-Evensen E, Bretthauer M, Gondal G, Vatn MH. Testing for faecal calprotectin (PhiCal) in the Norwegian Colorectal Cancer Prevention trial on flexible sigmoidoscopy screening: comparison with an immunochemical test for occult blood (FlexSure OBT). *Gut* 2004; 53: 1329-33. [CrossRef]
- Meucci G, D'Inca R, Maieron R, et al. Diagnostic value of faecal calprotectin in unselected outpatients referred for colonoscopy: A multicenter prospective study. *Dig Liver Dis* 2010; 42: 191-5. [CrossRef]
- Kok L, Elias SG, Witteman BJ, et al. Diagnostic accuracy of point-of-care fecal calprotectin and immunochemical occult blood tests for diagnosis of organic bowel disease in primary care: the Cost-Effectiveness of a Decision Rule for Abdominal Complaints in Primary Care (CEDAR) study. *Clin Chem* 2012; 58: 989-98. [CrossRef]
- Parente F, Marino B, Ilardo A, et al. A combination of faecal tests for the detection of colon cancer: a new strategy for an appropriate selection of referrals to colonoscopy? A prospective multicentre Italian study. *Eur J Gastroenterol Hepatol* 2012; 24: 1145-52. [CrossRef]
- Rutka M, Bor R, Balint A, et al. Diagnostic Accuracy of Five Different Fecal Markers for the Detection of Precancerous and Cancerous Lesions of the Colorectum. *Mediators Inflamm* 2016; 2016: 2492081. [CrossRef]
- Widlak MM, Thomas CL, Thomas MG, et al. Diagnostic accuracy of faecal biomarkers in detecting colorectal cancer and adenoma in symptomatic patients. *Aliment Pharmacol Ther* 2017; 45: 354-63. [CrossRef]
- Katsoula A, Paschos P, Haidich AB, Tsapas A, Giouleme O. Diagnostic Accuracy of Fecal Immunochemical Test in Patients at Increased Risk for Colorectal Cancer: A Meta-analysis. *JAMA Intern Med* 2017; 177: 1110-8. [CrossRef]
- Elias SG, Kok L, de Wit NJ, et al. Is there an added value of faecal calprotectin and haemoglobin in the diagnostic work-up for primary care patients suspected of significant colorectal disease? A cross-sectional diagnostic study. *BMC Med* 2016; 14: 141. [CrossRef]

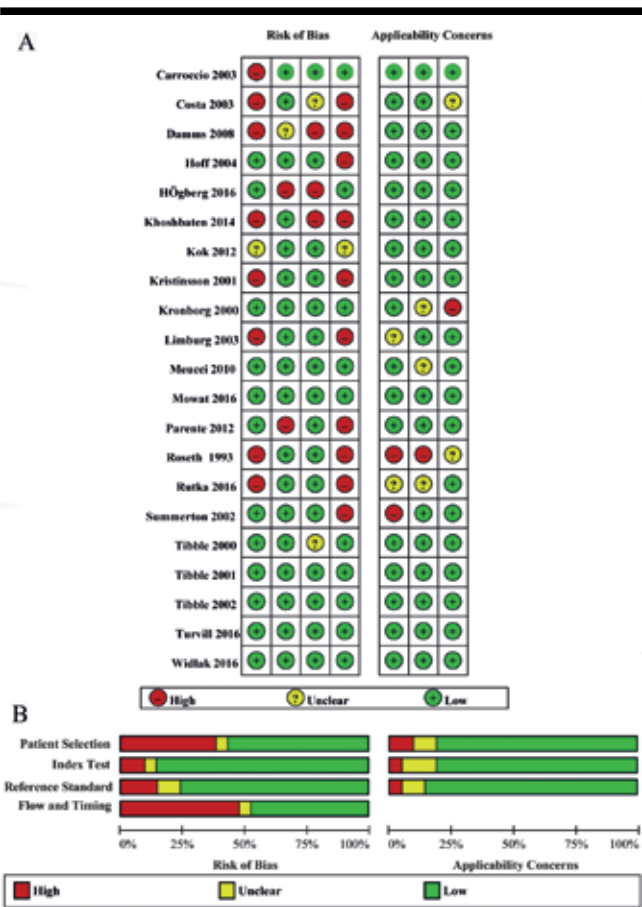


Figure S1. Risk of bias and applicability concerns: (A) Summary information (B) Graphical depiction

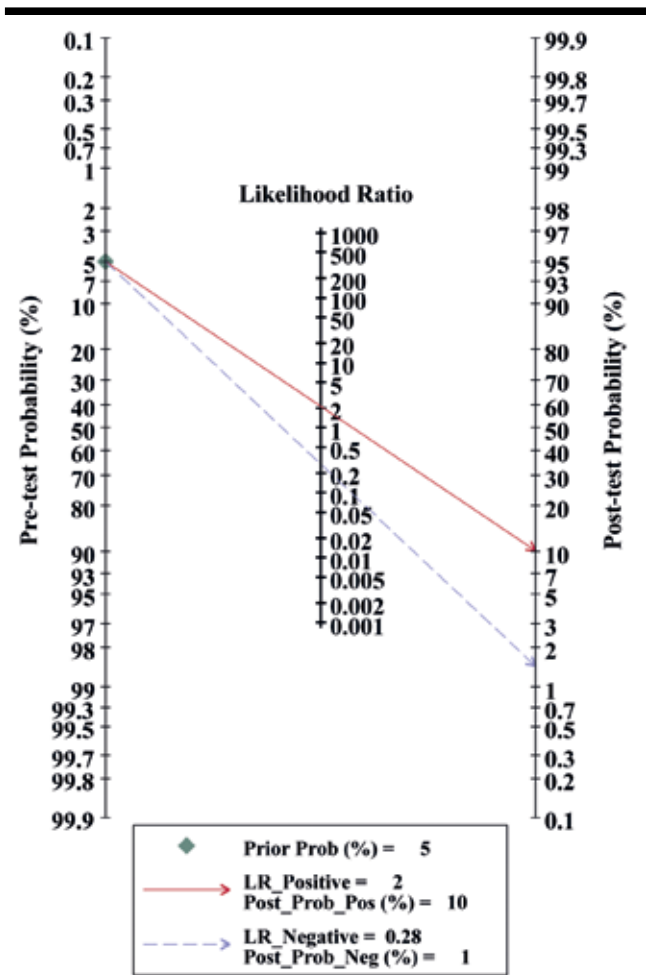


Figure S3. Fagan's plot for the post-test probability of CRC after an FC-positive result (upper line) or FC-negative result (lower line)

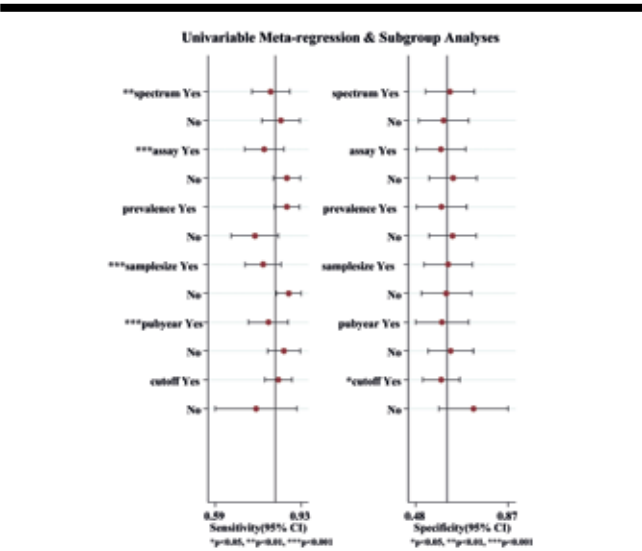


Figure S2. Meta-regression and subgroup analysis for sources of heterogeneity in CRC